

**GRASS TELEFACTOR**  
An Applied Medical Instrument Division

---

Home
Online Store
Contact Us
Site Map
Search

---

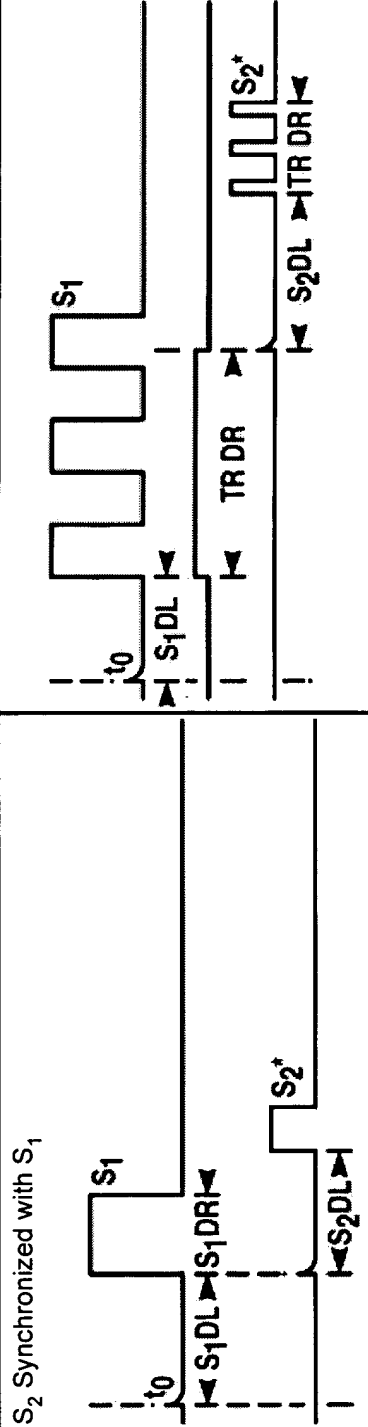
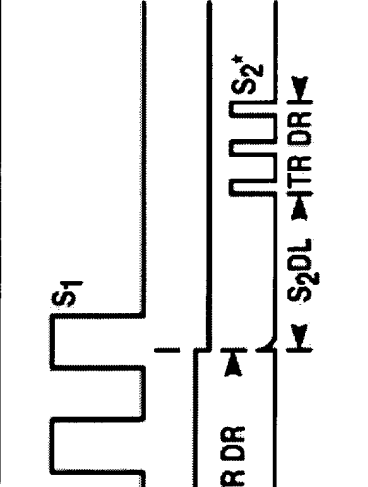
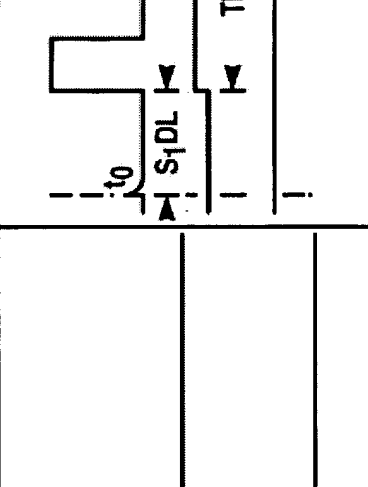
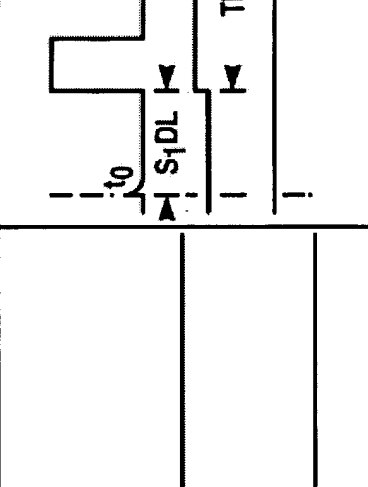
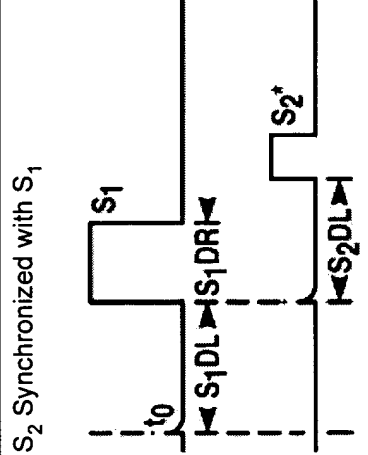
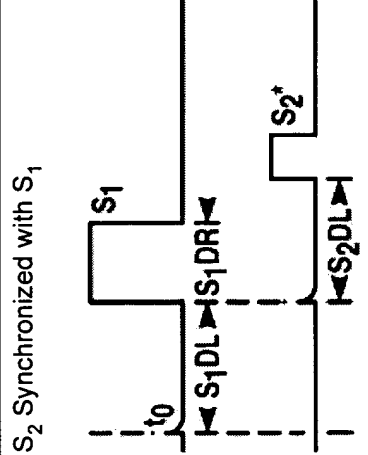
What's New?
Products
Service & Support
KnowledgeBase
Company

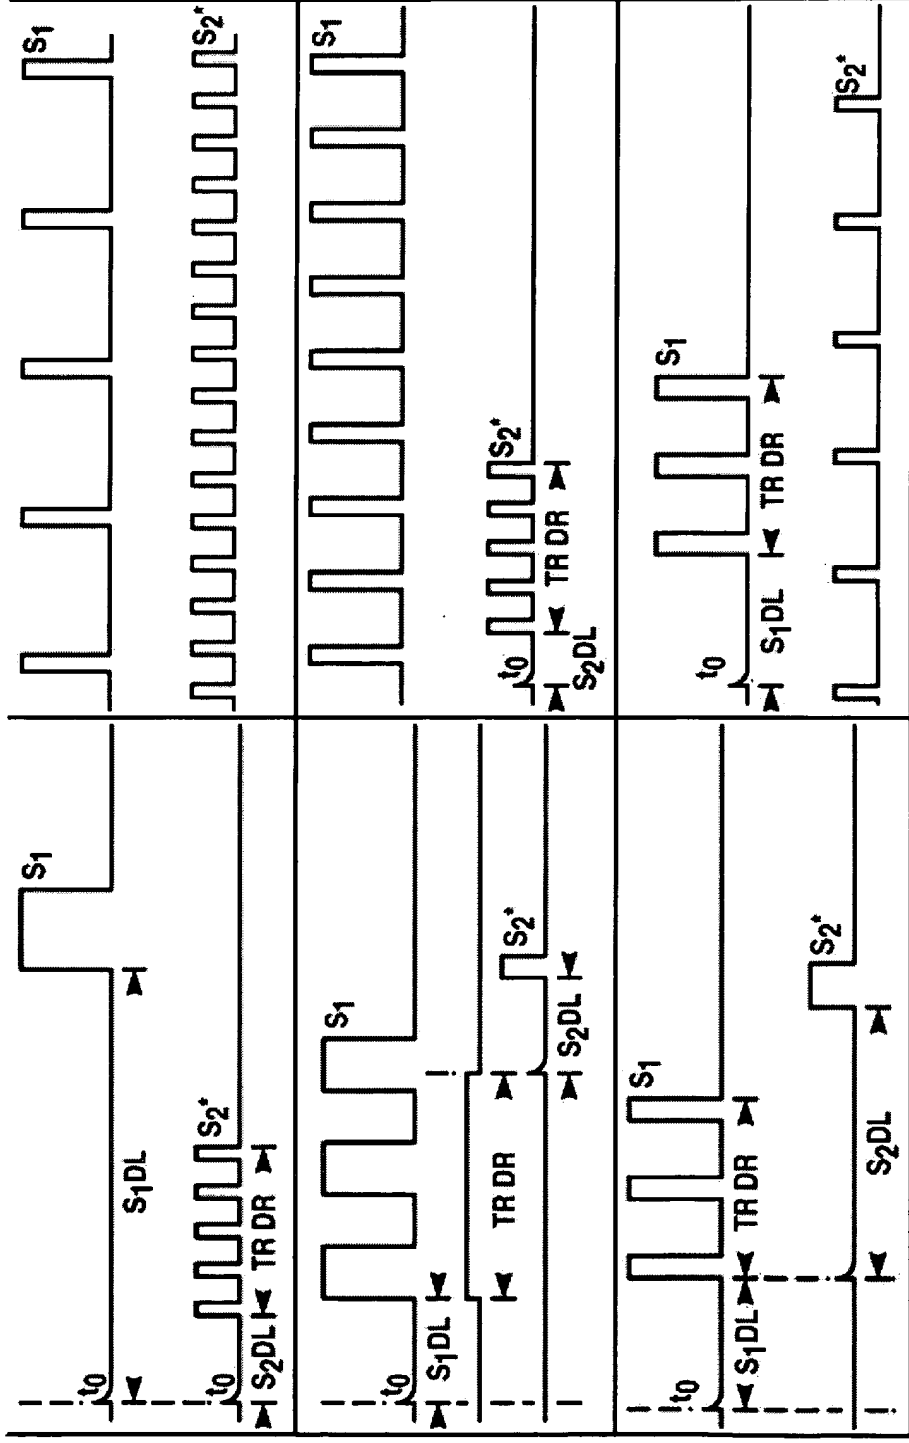
---

Wednesday, March 16, 2005

**S88 Stimulator Output Timing Patterns**

**Stimulators Table of Contents**

<p><math>S_2</math> Synchronized with <math>S_1</math></p> 	
	
	
<p><math>S_1</math> <math>S_2</math> Not Synchronized</p>	



← Previous Page

↑ Back To Top

Amplifiers | Amplifier Systems | Cabinets & Rack Carts | Cables & Connectors | Chart Paper & Recording Inks | Clinical Systems  
 Complete Systems | Direct Writing Recorders | Electrodes & Application Products | Maintenance | Research Software | Stimulators | Transducers

[Online Store](#) | [Ordering Information](#) | [Place An Order](#) | [Contact Us](#)

© 2005 Grass-Telefactor. All Rights Reserved.  
 An Astro-Med, Inc. Product Group

740